www.MDHearingAid.com

Printed in U.S.A.
09.13

MDHearingAid AIR®

THE DOCTOR'S CHOICE FOR AFFORDABLE HEARING AIDS®

User Manual

Congratulations!

As the owner of the MDHearingAid® AIR Hearing Aid, you may once again enjoy the sounds of your environment and conversations with your family and friends at a price you can afford. In order to get the most out of your MDHearingAid® AIR, please read this User Manual in its entirety. Your satisfaction with hearing aids depends on both the type and degree of your hearing loss as well as your expectations. No hearing aid can restore normal hearing, and not everyone will benefit equally.

Please read this manual in its entirety before using your MDHearingAid®AIR. Thank you!

Table of Contents

The MDHearingAid® Story . . . 2

Hearing Aid Diagram 4

Quick Start Guide 5

Package Contents 6

Fitting & Assembly

1. Select Ear Dome 8
2. Attach AIR Tubing 10
3. Insert Battery 11
4. Place Behind Ear 12
5. Turn Hearing Aid On 13

Selecting a Program 14

Phone/Telecoil Program 16

Getting the Most from Your Hearing Aid 18

Battery Information 22

Maintenance & Care 24

In Case of Malfunction 25

Troubleshooting 26

Replacement Parts 30

Warranty & Repair 31

Return Policy 32

Warnings 34

Important Notice for Prospective Users 36

Notice of Cancellation 38

Technical Specifications 39

The MDHearingAid® AIR Story

The MDHearingAid® AIR was invented by a board-certified Ear, Nose and Throat physician in Chicago, IL, Dr. Cherukuri. He encountered patients in his daily practice who would benefit from hearing aids, but many simply couldn't afford the thousands of dollars needed to pay for them. As a physician, he knew the effects of untreated hearing loss: depression, social isolation, anxiety, and other symptoms consistent with Alzheimer's disease.

Dr. Cherukuri set out to find a reasonable solution that could help with the most common types of hearing loss at a reasonable price. He was looking for a "one-size-fits-most" hearing aid, similar to reading glasses, that can easily be purchased at the drug store.

He evaluated numerous hearing aids and sound amplifiers, including those seen on television. He found almost all of these devices only amplified low frequencies (below 1000 Hz); however, the majority of hearing loss is in the higher frequencies (1000-4000 Hz), those most related to the human voice.

Dr. Cherukuri worked with world-class Doctors of Audiology and Audiologists to create the MDHearingAid® AIR. Built to exacting specifications, the MDHearingAid® AIR includes advanced technologies found on hearing aids costing thousands of dollars more such as:

- Advanced feedback cancellation to reduce and eliminate "whistling"
- Advanced compression technology to magnify soft sounds and dampen loud sounds
- Advanced noise reduction that reduces noises embedded in speech and maximizes sound quality
- Digital amplification to accurately reproduce speech and sounds to enhance listening comfort
- A Telecoil setting for easy use with compatible telephones or looped environments found in many churches, theatres and public buildings

The MDHearingAid® AIR has been rigorously tested by leaders in the hearing loss field (ENT Physicians and Audiologists) who have unanimously agreed that the sound quality and output is incredibly accurate.

MDHearingAid® AIR Diagram

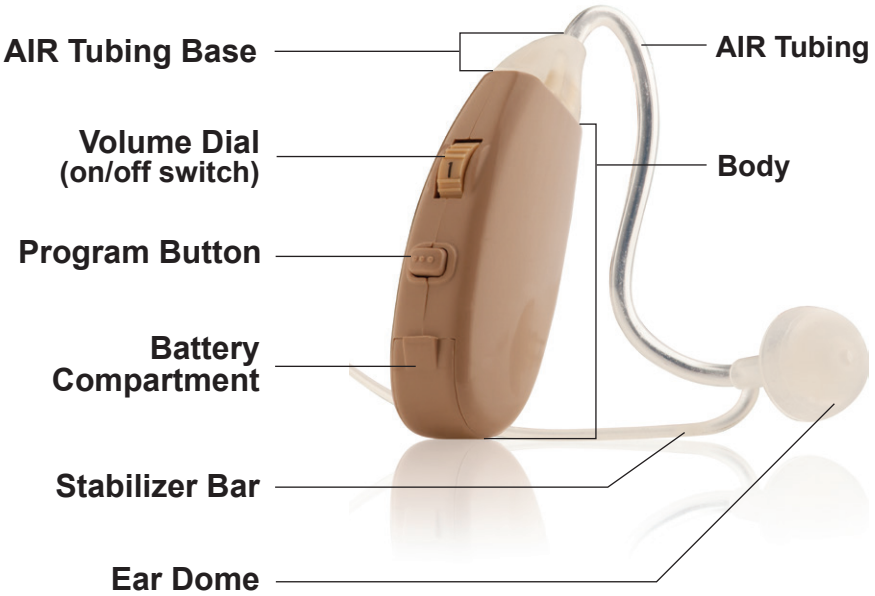

Quick Start Guide

Five Easy Steps for Fitting and Assembling Your MDHearingAid® AIR

Steps

Step 1: Select the Correct Ear Dome
Types: Open-Fit or Closed Ear Dome
Sizes: 6 mm – 15 mm

Step 2: Attach AIR Tubing Base to Hearing Aid Body

Step 3: Insert Battery

Step 4: Place Hearing Aid Behind Ear

Step 5: Turn the MDHearingAid® AIR On

MDHearingAid® AIR Package Contents

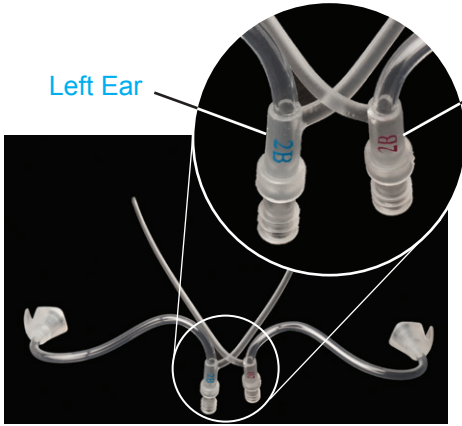

Right and Left ear AIR Tubing

- For Right ear, use the tubing labeled '2B' in Red
- For the Left ear use the tubing labeled '2B' in Blue.

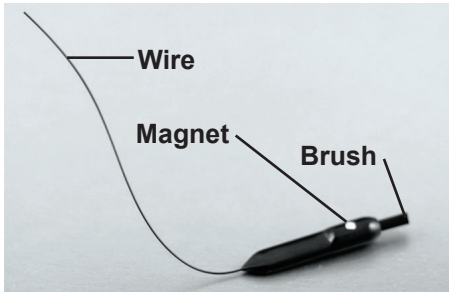

Cleaning Tool

Use Brush for removing wax around Ear Dome. Use the Magnet for replacement of battery. Use Wire to clean tubing (after removing Hearing Aid Body).

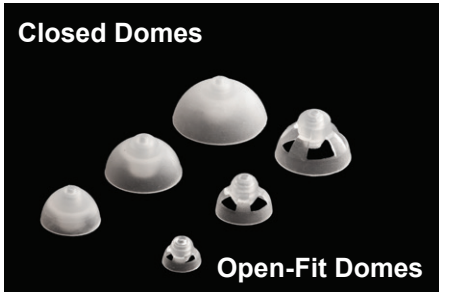

Ear Dome Selection

- Open-Fit Domes (vented) allow natural sound to enter the ear. Best for individuals who have high frequency loss and do not require high volume.
- Closed Domes are best for individuals who have low to high frequency loss or require higher volumes.

Optional Traditional Earhook System

This is ONLY for people needing maximum volume or a customized tubing length. (See separate package located under tray.)

Fitting and Assembly

Step 1: Select the Correct Ear Dome

Attach Ear Dome to AIR Tubing

Use Right AIR Tubing (Red lettering) for fitting Right ear. Use Left Tubing (Blue lettering) for fitting Left ear.

a) Hold the AIR Tubing at the junction of the Stabilizer Bar with one hand and hold the 'mushroom' top of the Ear Dome with the other hand.

b) Push the Ear Dome over the ridges on the end of the AIR Tubing.

c) Pull in the reverse direction to make sure the Ear Dome is attached securely.

Please note: while testing different Ear Dome sizes its best not to attach AIR Tubing to Hearing Aid Body.

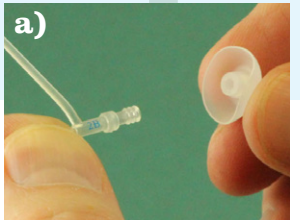

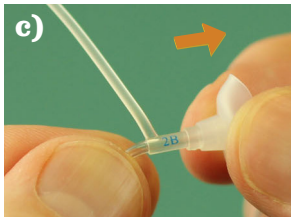

Insert Ear Dome in Ear Canal

a) Pull the outer ear upward and backward. With your other hand, hold the AIR Tubing (with Ear Dome attached) at the junction of the Stabilizer Bar.

b) Insert Ear Dome into the ear canal. It should fit in ear canal without protruding into the outer bowl of the ear. When the Ear Dome is too small, there is space between the Ear Dome and the ear canal, and you may hear whistling (feedback) when the Hearing Aid is on.

c) Nod head towards the ground to make sure that the Ear Dome does not slip out easily.

Repeat the 3 steps above with different sized Ear Domes to find the best one for you.



Step 2: Attach AIR Tubing Base to Hearing Aid Body

a) Hold the top of the AIR Tubing Base (the triangular end), and place it on the Hearing Aid Body's threaded end.

b) Twist the Hearing Aid Body clockwise, while gently pushing AIR Tubing Base onto threaded end of Hearing Aid Body.

c) Make sure the slots in the Base are flush with the wide sides of Hearing Aid Body.





Step 3: Insert Battery

To power up your Hearing Aid, please insert one of the included size 13 batteries.

a) Push the Nail Grip downward to open the Battery Compartment.

b) Remove the orange adhesive tab from the battery. With the red "+" side of Battery Compartment facing up, use the Cleaning Tool Magnet to insert the Battery.

Or, use orange adhesive tab to place battery in the Battery Compartment. Then remove adhesive tab and discard.

c) Close the Battery Compartment.

If the Battery Compartment does not close easily, the battery is inserted upside down.



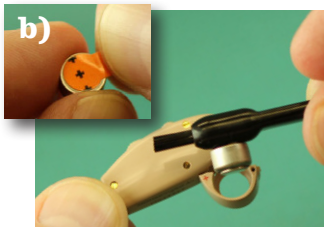

Step 4: Place Hearing Aid Behind Ear

a) Insert Ear Dome into the ear canal until the Ear Dome fits securely.
For more details see pictures on page 9.

b) Place the Hearing Aid Body behind the ear so the curve of the AIR Tubing rests comfortably on the top of ear in front of any eye wear.

c) Tuck the Stabilizer Bar in the outer bowl of the ear.

Please note: *The Stabilization Bar is often hidden when tucked in the outer bowl of the ear and is not shown on the cover of box.*

Step 5: Turn the MDHearingAid® AIR On

The MDHearingAid® AIR uses a Volume Dial with a built in on/off switch (like a radio).

- To turn the Hearing Aid **on**, turn the Volume Dial upward, past the click.
- To turn the Hearing Aid **off**, turn the Volume Dial downward until you feel a click.

IMPORTANT: *When the Hearing Aid is turned on, it will take a few seconds to begin amplifying sound. Please raise the volume SLOWLY to avoid sudden blast of sound.*

WARNING: *Whistling may be heard if the Hearing Aid is turned on but not positioned securely in your ear. This is normal. Once the Ear Dome is properly inserted in your ear, the whistling will stop.*

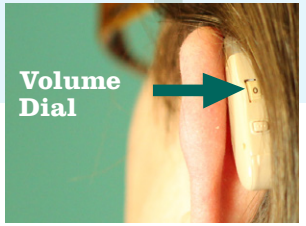

Selecting a Sound Processing Program

The MDHearingAid® AIR has four Sound Processing Programs to address the most common hearing loss environments. Try the different programs in each environment to find which Program works best for you.

- Once turned on, the MDHearingAid® AIR starts on Program 1.
  This is the default setting; every time the Hearing Aid is turned off and then on again, it will re-set to Program 1.
- To access the other Programs, press the Program Button and you will hear a number of audible tones corresponding to the Program number:

1 Tone = Program 1

2 Tones = Program 2

3 Tones = Program 3

4 Tones = Telecoil

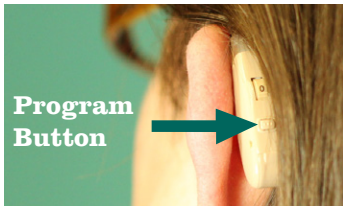

Please note: The tones may be faint depending on the volume setting and background noise.

Program	Best For	Description	Indicator
1. Normal Quiet Mode	Home, watching TV, time with family.	Increases sound in ALL frequencies.	1 Tone
2. Low Social Mode	Social settings: group meetings, church, time with friends.	Low frequencies (most background noises) up to 1000 Hz are not amplified.	2 Tones
3. High Noisy Mode	Intense noise situations: parties, restaurants, traffic or large crowds. Ideal for people with high frequency hearing loss.	Frequencies up to 1500 Hz are not significantly amplified.	3 Tones
4. Telecoil	Use with compatible telephones and looped environments (pg. 16).	Telecoil enabled. Microphone is off.	4 Tones

Using the Telephone/Telecoil Program

The MDHearingAid® AIR is equipped with a Telecoil Program. Telecoils, also known as an Audio Induction Loops, enable the direct magnetic coupling of your Hearing Aid to compatible telephones and other audio sources.

Telecoils provide clear sound that is free of background noise and feedback. Telecoils enable you to comfortably use the telephone without removing your Hearing Aid.

To activate the Telecoil mode (Program 4)

Push the Program Button until you hear four tones. In Telecoil mode, the Hearing Aid microphone is disabled; only the sounds picked up from the Telecoil are amplified.

General Telephone Use

When using the Telecoil, be sure to center the telephone receiver over the Hearing Aid, NOT your ear canal. Move the receiver along the Hearing Aid to locate the clearest, strongest signal. You may have to increase the volume of the Hearing Aid slightly. To return to normal listening, push the Program Button until the desired program is reached.

Telephone Compatibility

Most, but not all, landline phones are Telecoil compatible. Wireless and cellular phones rated T3 or T4 are Telecoil compatible (T4 is preferred). Check your telephone's instruction manual to find out its rating.

Phones rated M3 or M4 are not Telecoil compatible but are hearing aid compatible. These phones will work with programs 1-3.

The speaker function on your phone also works well with your MDHearingAid® Hearing Aids.

Compatible Loop Systems

The Telecoil Program can also help you listen in public places equipped with Telecoil compatible assisted listening systems. If your Hearing Aids do not operate when the Telecoil is on, the loop system may not be operating or you may be in a "dead" spot. Try positioning yourself in a different part of the looped area, or return your Hearing Aids to your preferred Program 1-3 and sit as close to the speaker as possible.

Getting the Most from Your Hearing Aid

Your satisfaction with Hearing Aids depends on the type and degree of your hearing loss and your expectations. No hearing aids will restore the normal hearing of youth, including those costing thousands of dollars.

However, you can maximize your return on your investment by understanding the 3 Keys to Hearing Aid Happiness.

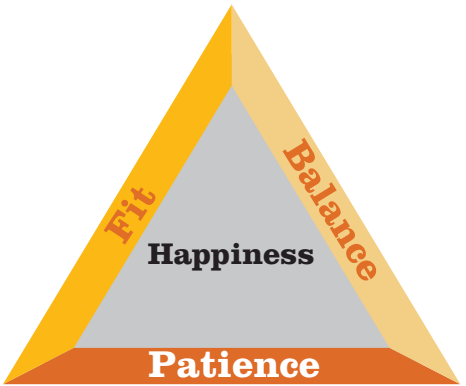

Key #1 — Patience

New hearing aids can be a big adjustment. Your brain has to re-learn how to hear and listen. After many years of not hearing well, it takes time and practice to redevelop these skills. Medical studies show that your brain requires approximately 21 days to adjust to your new Hearing Aids. During this time:

- You may initially notice lots of background sounds. These sounds have always been a part of your environment. In time your brain will re-learn how to process these sounds by prioritizing foreground over background sounds.
- You may find that a quiet environment is more comfortable in the beginning of the adjustment period.
- Your voice may sound too loud. This effect is very common for new hearing aid users, but most people get used to it over time.
- You voice may also sound 'plugged up' or like you're talking in a barrel. This occlusion effect is normal. The sensation usually goes away in the first few weeks.
- In noisy environments, you may find it easier to understand speech by facing the speaker. Reading lips and observing facial expressions and body language reinforce the sound communication.

Key #2 — Fit

Hearing Aids, no matter how expensive, are almost useless if they don't fit well. Without a proper fit, it is impossible to reap the full benefit of your investment.

- Your Hearing Aids comes with six different silicone Ear Domes. Choose the appropriate size Ear Dome for your ear so that the fit inside the ear canal is snug. If the fit is loose, feedback will occur, and you may hear a whistling noise when the Hearing Aids are on.
- It can take time for Hearing Aids to feel comfortable. Try wearing them for 30-60 minutes a day at first and gradually extend the amount of time that you wear them.
- You may find that you require a different Ear Dome size or type once your ear has adjusted to wearing Hearing Aids regularly.

Using Hearing Aids takes practice and patience. Some people adjust very quickly and most adapt within a few weeks. Please do not give up prematurely. A whole new world of sound awaits you.

Key #3 — Balance

We are born with two ears for balance. It is best to maintain balance while treating hearing loss. If you have hearing loss in both ears, medical studies have shown that **You will get far greater satisfaction and the BEST results by wearing two Hearing Aids**, for the following reasons:

- You will have a significantly better understanding of speech and conversation, since the brain is receiving a balanced signal from both ears.
- You will find there will be less overall background noise amplification.
- You will have better hearing and understanding in noisy situations.
- You will have better localization of the direction of sounds.
- Your listening will be more pleasing, effortless, and less frustrating.

If you have hearing loss in both ears and only ordered one Hearing Aid, we strongly encourage you to use the enclosed coupon for a discount on a second MDHearingAid® AIR. As always, you will receive a 45-day risk-free trial with our money-back guarantee.

Important Battery Information

Low Battery Warning

When the battery voltage nears the end of its life, the MDHearingAid® AIR will provide a low battery warning signal. The initial warning will be three sets of double beeps. At this point, the hearing aid is still functioning, but it is recommended that the battery be replaced as soon as possible.

When the battery is too weak for further operation, the MDHearingAid® AIR will issue six sets of double beeps (resembling a motor boat sound) and then shut down all audio output of the Hearing Aid. At this point, the unit will not function until a fresh battery is installed.

Do not leave exhausted "dead" batteries in the Hearing Aid, as they may leak and damage the Hearing Aid. Discard/Recycle the exhausted batteries.

***Caution!** Batteries can be harmful if swallowed. Keep batteries out of reach of children and pets. If a battery is accidentally swallowed, seek medical attention immediately, or call the **National Battery Hotline collect at 202-625-3333**.*

Battery Type:

The MDHearingAid® AIR uses size **13/13A zinc-air batteries.**

Battery Expiration Location:

Found on back of battery package.



Battery Life:

Depends on a number of factors, such as the settings of your Hearing Aids and the number of hours used per day.

For extended battery life, open the Battery Compartment if the Hearing Aid will not be used for a prolonged period of time. This can be performed every night, after removal, before going to sleep.



Battery Removal:

Hold the Hearing Aid over a table, then turn the Hearing Aid over, and battery will fall out.
Please Recycle exhausted batteries.

Maintenance & Care Suggestions

Follow these tips to keep your MDHearingAid® AIR performing optimally:

- Wipe your Hearing Aid daily with a tissue or soft cloth. Water, alcohol, or other liquid agents will damage it.
- Keep your ears clean to maximize the benefit of your MDHearingAid® AIR. Earwax can clog up AIR Tubing. For best results, it may be beneficial to clean your ears with an over-the-counter ear wash kit or visit your physician.
- Use the wire on the Cleaning Tool to keep AIR Tubing free from debris.
- Use the brush on the Cleaning Tool to gently clean away wax and other debris.
- Do not let the Hearing Aid get wet. Do not use hair spray or a hair dryer while wearing the Hearing Aid. Do not expose the Aid to excess moisture or heat.
- Avoid physical shock to the Hearing Aid, such as dropping it on the floor.
- Store your Hearing Aid in a cool dry place when not in use with the Battery Compartment door open.
- If you are not going to use the Hearing Aid for a prolonged period of time, remove the battery to prevent corrosion.

In Case of Malfunction

Should your Hearing Aid not function properly, try the following:

1. Make sure the Hearing Aid is switched on.
2. Change the battery and make sure the new battery is inserted correctly.
3. Check that the Ear Dome or AIR Tubing is not blocked by earwax.
4. Disconnect the AIR Tubing from the hearing aid and check for moisture in the AIR Tubing.
5. Read the Troubleshooting guide on the following pages.
6. Check the website **www.mdhearingaid.com/customer-service/** for more Troubleshooting tips.

Troubleshooting

1. Instrument makes a whistling sound.

- Whistling (feedback) occurs when amplified sound returns to the microphone and is re-amplified. Most hearing aids (even ones costing thousands of dollars) will whistle when not inserted properly in the ear canal.
- Lower the volume if it is set too high, and try using a non-vented Closed Ear Dome.
- Clean any wax from the AIR Tubing that may be interfering with the Hearing Aid.
- If feedback is still an issue try using the Traditional Earhook System.
- Confirm that the Hearing Aid is working properly by removing the aid and covering the end of the AIR Tubing or attached Ear Dome with your finger. The whistling should stop.
- Try reinserting the Ear Dome into ear so it fits better. If that doesn't work, try a different size Ear Dome.
- Occasionally, whistling may occur when you have a blockage of wax in the ear canal from a cold or any condition that causes sound to be reflected from the ear canal. In these cases, the fit may be fine and the whistling will disappear when the condition is corrected.
- Check for cracks in the AIR Tubing or Base. Cracks may become another entrance for sound to enter and cause feedback.

For optimal performance, the Hearing Aid Ear Domes and AIR Tubing should be replaced every 3-6 months. Replacements can be ordered at: **www.mdhearingaid.com/accessories.**

2. The sound is distorted or intermittent.

- If the hearing aid were in a humid environment or subject to sweat, moisture may clog the aid and distort sounds. Consider using a hearing aid dehumidifier overnight.
- Lower the volume.
- Replace battery with a fresh one.
- Check the Ear Domes and AIR Tubing for wax or for any signs of wear. Replace the Ear Domes and AIR Tubing if they appear stiff, bent, cracked, or frayed. Replacements can be ordered at: **www.mdhearingaid.com/accessories**.

3. Instrument has a weak or no sound.

- Make sure the Hearing Aid is on. The Volume Dial should be set above the number 1.
- Make sure battery is fresh. If there is any doubt, try a new battery.
- Make sure battery is inserted correctly and Battery Compartment is completely closed.
- Reposition the AIR Tubing and Ear Dome in your ear canal.
- Rotate the Volume Dial (on/off switch) back and forth, in case dust or lint has collected in the controls.

Replacement of AIR Tubing & Ear Domes

For OPTIMAL PERFORMANCE, the AIR Tubing and Ear Domes should be replaced every 3-6 months:

- Over time, AIR Tubing and Ear Domes may become stiff and discolored.
- Regular replacement keeps your hearing aids sounding and feeling like new.
- Visit **www.mdhearingaid.com/shop/accessories** where we offer different sizes of replacement Ear Domes and Tubing if you are having difficulty achieving a proper fit.

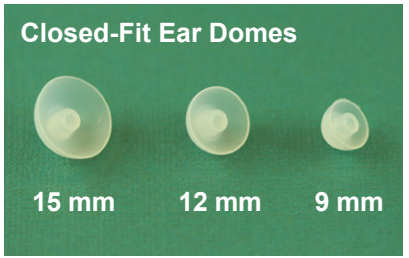

Warranty & Repair

The MDHearingAid® AIR is covered against defects in materials and workmanship for 90 days from the date you receive your order. If our examination determines that the unit failed to work due to parts, materials or workmanship, we will repair or replace it for free. *This warranty does not cover malfunctions due to unusual wear and tear or mistreatment of the Hearing Aid, such as physical shock, damage from moisture or sweat, excessive wax build-up, or tampering with the instrument, all of which void the warranty.*

If you require **Warranty or Repair Service,** please contact Customer Service for a Return Merchandise Authorization (RMA) number, repair costs, and instructions.

For fastest service e-mail:
support@mdhearingaid.com

Or, call Customer Service at:
312-219-8422. Office hours:
Monday to Friday,
8:30 am to 4:30 pm (CST).

Repair Facility address:
MDHearingAid, Inc.
Repairs Department
18447 W. 8 Mile Road
Detroit, MI 48219-1520

Please do not mail to this address without contacting Customer Service first.

Return Policy

At MDHearingAid® your satisfaction is **guaranteed.**

To get the most out of your MDHearingAid® AIR Hearing Aids, please understand that no hearing aid will restore normal hearing. Your satisfaction with the MDHearingAid® AIR depends to some degree on your expectations and commitment to re-training your brain how to hear and listen.

45 Day Trial Period

You have 45 days from the date of purchase to return the hearing aids. The reason for this long trial period is that often it takes several weeks to get used to the sound of new hearing aids (even the most expensive ones).

21 Day Refund Policy

Medical studies show that your brain requires approximately 21 days to adjust to new hearing aids. **If, after 21 days of using the MDHearingAid® AIR (and before the 45th day from purchase), you are still not satisfied, please contact us for a RMA number.**

You will receive a **full refund** of your purchase price less shipping costs (or as directed by the site where you made the purchase). Detailed return instructions will be explained over the phone or can be e-mailed to you along with your RMA number.

For fastest service, please e-mail **support@mdhearingaid.com**. Alternatively, you may call **312-219-8422.** Customer Support office hours are Monday to Friday, 8:30am to 4:30pm Central Standard Time.

Restocking Fees

Requests for an RMA number **prior to trying** the hearing aid(s) for 21 days will be granted but will carry a 10% restocking fee. Returns made without a RMA number will incur a twenty percent (20%) restocking fee.

We are sorry, but we are unable to honor return requests after 45 days from the date of purchase.

Warnings to Hearing Aid Dispensers

A hearing aid dispenser should advise a prospective hearing aid user to consult promptly with a licensed physician (preferably an ear specialist) before dispensing a hearing aid. If the hearing aid dispenser determines through inquiry, actual observation, or review of any other available information concerning the prospective user, that the prospective user has any of the following conditions, then consult a physician.

- Visible congenital or traumatic deformity of the ear.
- History of active drainage from the ear within the previous 90 days.
- History of sudden or rapidly progressive hearing loss within the previous 90 days.
- Acute or chronic dizziness.
- Pain or discomfort in the ear.
- Unilateral hearing loss of sudden or recent onset within the previous 90 days.
- Audiometric air-bone gap equal to or greater than 15 decibels at 500 hertz (Hz), 1000 Hz, and 2000 Hz.
- Visible evidence of significant cerumen accumulation or a foreign body in the ear canal.

Stop Using MDHearingAid® AIR and Consult a Physician if:

- Hearing in one or both ears worsens.
- Hearing does not improve while using the MDHearingAid® AIR
- Skin irritation develops in or around your ear canal.
- Your ear becomes occluded with excessive ear wax.
- You develop an infection of your ear or ear canal.

Special care should be exercised in selecting and fitting a hearing aid whose maximum sound pressure level exceeds 132 decibels because there may be risk of impairing the remaining hearing of the hearing aid user.

A hearing aid will not restore normal hearing and will not prevent or improve a hearing impairment resulting from organic conditions. In most cases infrequent use of a hearing aid does not permit a user to attain full benefit from it. The use of hearing aid(s) is only part of hearing rehabilitation and may need to be supplemented by auditory training and instruction in lip reading.

Important Notice for Prospective Users

Good health practice requires that a person with a hearing loss have a medical evaluation by a licensed physician (preferably a physician who specializes in diseases of the ear) before purchasing a hearing aid. Licensed physicians who specialize in diseases of the ear are often referred to as otolaryngologists, otologist or otorhinolaryngologists. The purpose of a medical evaluation is to assure that all medically treatable conditions that may affect hearing are identified and treated before the hearing aid is purchased.

Following the medical evaluation, the physician will give you a written statement that your hearing loss has been medically evaluated and you may be considered a candidate for a hearing aid. The physician will refer you to an audiologist or a hearing aid dispenser, as appropriate, for a hearing aid evaluation.

The audiologist or hearing aid dispenser will conduct a hearing aid evaluation to assess your ability to hear with and without a hearing aid. The hearing aid evaluation will enable the audiologist or dispenser to select and fit a hearing aid suited to your individual needs.

If you have reservations about your ability to adapt to amplification, you should inquire about the availability of a trial/rental or purchase/option program. Many hearing aid dispensers now offer programs that permit you to wear a hearing aid for a period of time for a fee after which you may decide if you want to purchase the hearing aid.

Federal law restricts the sale of hearing aids to those individuals who have obtained a medical evaluation from a licensed physician. Federal law permits a fully informed adult to sign a waiver statement declining the medical evaluation for religious or personal beliefs that preclude consultation with a physician. The exercise of such a waiver (without prior consultation by an ear specialist) is not in your best health interest, and its use is strongly discouraged.

Children with hearing loss

This product is not for use by anyone under 18 years of age. In addition to seeing a physician for a medical evaluation, a child with a hearing loss should be directed to an audiologist for evaluation and rehabilitation. Hearing loss may cause problems in language development, educational growth, and social growth of a child. An audiologist is qualified by training and experience to assist in the evaluation and rehabilitation of a child with a hearing loss.

Notice of Cancellation

YOU MAY CANCEL THIS TRANSACTION, WITHOUT ANY PENALTY OR OBLIGATION, AFTER 21 DAYS AND BEFORE 45 DAYS FROM THE DATE OF PURCHASE. IF YOU CANCEL, ANY PROPERTY TRADED IN, ANY PAYMENTS MADE BY YOU UNDER THE CONTRACT OR SALE LESS ANY NONREFUNDABLE RESTOCKING FEE, AND ANY NEGOTIABLE INSTRUMENT EXECUTED BY YOU WILL BE RETURNED WITHIN 10 BUSINESS DAYS FOLLOWING RECEIPT BY THE SELLER OF YOUR CANCELLATION NOTICE AND ALL MERCHANDISE PERTAINING TO THIS TRANSACTION, AND ANY SECURITY INTEREST ARISING OUT OF THE TRANSACTION WILL BE CANCELLED. IF YOU CANCEL, YOU MUST RETURN TO THE SELLER, IN SUBSTANTIALLY AS GOOD CONDITION AS WHEN RECEIVED, ANY GOODS DELIVERED TO YOU UNDER THIS CONTRACT OR SALE. TO CANCEL THIS TRANSACTION, MAIL OR DELIVER A SIGNED AND DATED COPY OF THIS CANCELLATION NOTICE OR ANY OTHER WRITTEN NOTICE, OR SEND A TELEGRAM, TO MDHEARINGAID, 917 W. WASHINGTON BLVD, SUITE 202, CHICAGO, IL 60607 NO LATER THAN MIDNIGHT OF THE 45TH DAY AFTER THE INITIAL TRANSACTION. “I HEREBY CANCEL THIS TRANSACTION,” SIGNED:

_____ (Buyer’s Signature)

_____ (Date)

Technical Specifications

MAX OSPL90	126 dBSPL
HF Average OSPL90	119 dBSPL
HFA Full-on-gain	40 dBSPL
THD@	800 Hz. 0.6%
	1600 Hz 0.7%
EQUIV INPUT NOISE	26 dB
BATTERY CURRENT DRAIN	0.90 mA